


Traceability scheme - CSM Temperature lab

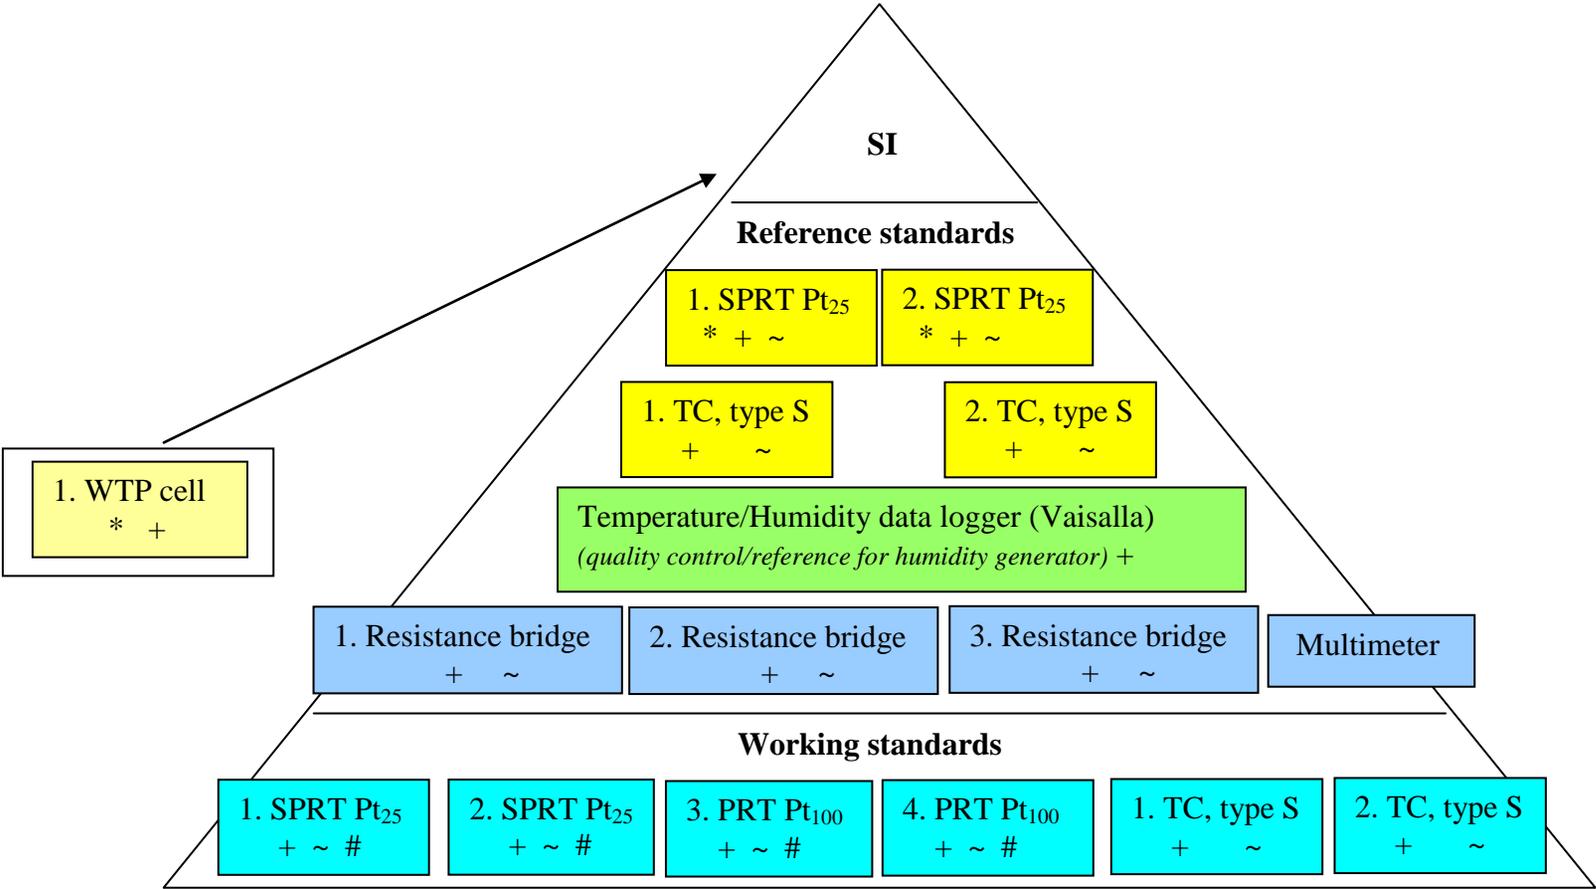

* calibration at NMI, listed at BIPM data base for the required measuring range (when application for CMC entries intended)
 + calibration at calibration laboratory, accredited according to ISO/IEC 17025 for the required measuring range (DAkkS,NVLAP)
 # internal calibration (when accredited)
 ~ intermediate check (SPRT / PRT at water triple point, resistance bridge with standard resistors)

Laboratory of national standards of CSM under ME KR		Edition #	3
P 6.5_ A1/02	Traceability matrix	Date of issue	30.04.2019
		Page	2 from 2

Date	30.04.2019	Version	3	Update made by	Denisova
-------------	------------	----------------	---	-----------------------	----------